

ThreeSide Peptides
 10600 Endeavour Way Suite 3
 Largo, FL 33777



Project 135679
Lab # 132069
Date Rec'd 1/7/2026
Report Issued 1/20/2026

Project

Sample hCG 5000 IU HCG5K2512

Certificate of Analysis



<u>Analyte</u>	<u>Result</u>	<u>LOQ</u>	<u>Units</u>	<u>% of Label</u>	<u>Method</u>	<u>Date</u>	<u>CAS</u>
Peptide Analysis							
Chromatographic purity	98.49	0.5	%		HPLC-UV/MS	1/14/2026	
hCG	4,680	0.5	IU	93.6	HPLC-UV-MS	1/14/2026	9002-61-3
hCG	ID Confirmed				HPLC-UV-MS	1/14/2026	

The data presented are from the analysis of the sample shown and meet Krause Analytical internal quality assurance criteria unless otherwise flagged.
 Methods shown reference current Krause Analytical SOPs
 ND - Not detected LOQ - limit of quantification
 Copyright © 2025 Krause Analytical LLC. All rights reserved.

Respectfully submitted,


Mark C. Krause
 Laboratory Director



krause analytical

Chromatogram

Response_

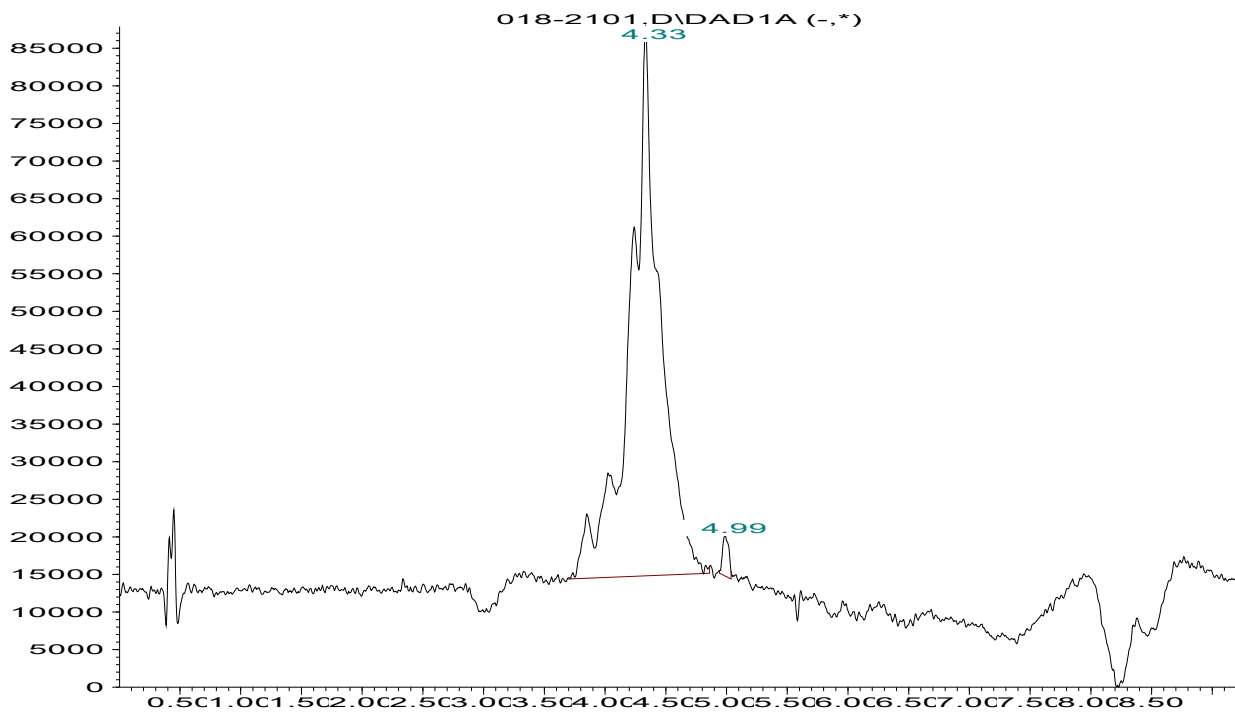

Time

Mass spectrum/Reference Spectrum

Concentration of the peptide in solution is too low to obtain a valid mass spectrum for this sample